

9290-10

クランプオンアダプタ CLAMP ON ADAPTER

取扱説明書 / Instruction Manual

2013年9月 改訂5版 Printed in Japan
9290B980-05 13-09H



HIOKI

日置電機株式会社

■ 製品のお問い合わせはコールセンターまで

☎0120-72-0560 9:00～12:00,13:00～17:00
土・日・祝日を除く

TEL **0268-28-0560** FAX 0268-28-0569 E-mail info@hioki.co.jp

■ 修理・校正のご依頼はお買上店（代理店）または最寄りの営業所まで
また、ご不明な点がございましたらサービスお問合せ窓口まで
TEL 0268-28-0823 FAX 0268-28-0824 E-mail cs-info@hioki.co.jp

■ お問い合わせ・販売ネットワーク

<http://www.hioki.co.jp/contact/>



本社 〒386-1192 長野県上田市小泉 81
TEL 0268-28-0555 FAX 0268-28-0559

1308

保証書		HIOKI					
形名	9290-10	製造番号	保証期間 購入日 年 月 日より 1年間				
<p>本製品は、弊社の厳密な検査を経て合格した製品をお届けした物です。万一ご使用中に故障が発生した場合は、お買い求め先にご連絡ください。本書の記載内容で無償修理をさせていただきます。また、保証期間は購入日より1年間です。購入日が不明の場合は、製品の製造年月から1年を目安とします。ご連絡の際は、本書を提示してください。また、確度については、明示された確度保証期間によりります。</p> <p>お客様 住所: 〒 _____ ご芳名: _____</p> <p>*お客様へのお断り 保証書の再発行はいたしませんので、大切に保管してください。 「製造番号」購入日、およびお客様「ご住所、ご芳名」は恐れ入りますが、お客様にて記入していただきますようお願いいたします。</p> <p>1. 取扱説明書・本体注意ラベル（刻印を含む）等の注意事項に従った正常な使用状態で保証期間内に故障した場合には、無償修理いたします。また、製品のご使用による損失の補償請求に対しては、弊社善後の上購入金額までの補償とさせていただきます。 なお、製造後一定期間を経過したものとおよび部品の生産中止、不測の事態の発生等により修理不可能となった場合は、修理、校正等を辞退する場合がございます。</p> <p>2. 保証期間内でも、次の場合には保証の対象外とさせていただきます。</p>							
<p>-1. 製品を使用した結果生じる被測定物の、二次的、二次的な損傷、被害 -2. 製品の測定結果がもたらす、二次的、二次的な損傷、被害 -3. 取扱説明書に基づかない不適当な取り扱い、または使用による故障 -4. 弊社以外による修理や改造による故障および損傷 -5. 取扱説明書に明示されたものを含む部品の消耗 -6. お買い上げ後の輸送、落下等による故障および損傷 -7. 外観上の変化（筐体のキズ等） -8. 火災、風水害、地震、落雷、電源異常（電圧、周波数等）、戦争・暴動行為、放射能汚染およびその他天災地変等の不可抗力による故障および損傷 -9. 各種通信・ネットワーク接続による損害 -10. 保証書の提出が無い場合 -11. その他弊社の責任とみなされない故障 -12. 特殊な用途（宇宙用機器、航空用機器、原子力用機器、生命に関わる医療用機器および車輛制御機器等）に組み込んで使用する場合で、もってその旨を連絡いただかない場合</p> <p>3. 本保証書は日本国内のみ有効です。 (This warranty is valid only in Japan.)</p>							
<p>サービス記録</p> <table border="1"> <thead> <tr> <th>年月日</th> <th>サービス内容</th> </tr> </thead> <tbody> <tr> <td> </td> <td> </td> </tr> </tbody> </table>				年月日	サービス内容		
年月日	サービス内容						
<p>日置電機株式会社 〒386-1192 長野県上田市小泉 81 TEL 0268-28-0555 / FAX 0268-28-0559 10-09</p>							

はじめに

このたびは、HIOKI 9290-10 クランプオンアダプタをご選定いただき、誠にありがとうございます。この製品を十分にご活用いただき、末長くご使用いただくために、取扱説明書はていねいに扱い、いつも手元に置いてご使用ください。

概要

9290-10 クランプオンアダプタは、AC1500 A 定格、CT 比 10:1 のクランプアダプタです。広い周波数特性や良好な位相特性を兼ね備えており、クランプセンサだけでなく、クランプオンパワーハイテスタなどのレンジ拡大、大電流測定を可能にします。

点検

本器がお手元に届きましたら、輸送中において異常または破損がないか点検してからご使用ください。万一、破損あるいは仕様と異なる動作しない場合は、お買上店（代理店）か最寄りの営業所にご連絡ください。

保守・サービス

- 本器の汚れをとるときは、柔らかい布に水か中性洗剤を少量含ませて、軽く拭いてください。ベンジン、アルコール、アセトン、エーテル、ケトン、シンナー、ガソリン系を含む洗剤は絶対に使用しないでください。変形変色することがあります。
- 故障と思われるときは、お買上店（代理店）か最寄りの営業所にご連絡ください。輸送中に破損しないように梱包し、故障内容も書き添えてください。輸送中の破損については保証しかねます。

安全について

本器を安全にご使用いただくために、また機能を十二分に活用いただくために、下記の注意事項をお守りください。

⚠ 危険

この機器は IEC 61010 安全規格に従って、設計され、試験し、安全な状態で出荷されています。測定方法を間違えると人身事故や機器の故障につながる可能性があります。取扱説明書を熟読し、十分に内容を理解してから操作してください。万一事故があっても、弊社製品が原因である場合以外は責任を負いかねます。

安全記号

	使用者は、取扱説明書内の ⚠ マークのあるところは、必ず読み注意する必要がありますを示します。使用者は、機器上に表示されている ⚠ マークのところについて、取扱説明書の ⚠ マークの該当箇所を参照し、機器の操作をしてください。
	二重絶縁または強化絶縁で保護されている機器を示します。
	交流 (AC) を示します。
	活線状態の電路に着脱できることを示します。

取扱説明書の注意事項には、重要度に応じて以下の表記がされています。

⚠ 危険 操作や取扱いを誤ると、使用者が死亡または重傷につながる危険性が極めて高いことを意味します。

⚠ 警告 操作や取扱いを誤ると、使用者が死亡または重傷につながる可能性があることを意味します。


⚠ 注意 操作や取扱いを誤ると、使用者が傷害を負う場合、または機器を損傷する可能性があることを意味します。

注記 製品性能および操作上でのアドバイスのことを意味します。

測定カテゴリについて

本器は CAT III に適合しています。測定器を安全に使用するため、IEC61010 では測定カテゴリとして、使用する場所により安全レベルの基準を CAT II ~ CAT IV で分類しています。

- CAT II:** コンセントに接続する電源コード付き機器（可搬形工具・家庭用電気製品など）の一次側電路
コンセント差込口を直接測定する場合は CAT II です。
- CAT III:** 直接分電盤から電気を取り込む機器（固定設備）の一次側および分電盤からコンセントまでの電路
- CAT IV:** 建造物への引込み電路、引込み口から電力量メータおよび一次側電路保護装置（分電盤）までの電路

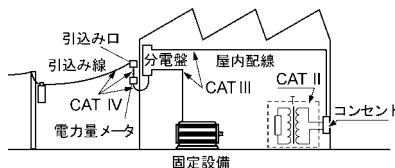

カテゴリの数値の小さいクラスの測定器で、数値の大きいクラスに該当する場所を測定すると重大な事故につながる恐れがありますので、絶対に避けてください。カテゴリのない測定器で、CAT II ~ CAT IV の測定カテゴリを測定すると重大な事故につながる恐れがありますので、絶対に避けてください。

使用上の注意



この取扱説明書には本器を安全に操作し、安全な状態に保つのに要する情報や注意事項が記載されています。本器を使用する前に下記の安全に関する事項をよくお読みください。

⚠ 危険

- 短絡事故や人身事故を避けるため、本器は AC600 V 以下の電路で使用してください。
- 本器は、必ずプレーカの二次側に接続してください。プレーカの二次側は、万一短絡があっても、プレーカにて保護します。一次側は、電流容量が大きく、万一短絡事故が発生した場合、損傷が大きくなるので、測定しないでください。
- 感電事故を防ぐため、使用中はバリア（障壁）より先を触らないでください。

⚠ 警告

- 本器をぬらしたり、ぬれた手で測定しないでください。感電事故の原因になります。
- 活線で測定するので、感電事故を防ぐため、労働安全衛生規則に定められているように、電気用ゴム手袋、電気用ゴム長靴、安全帽等の絶縁保護具を着用してください。
- 測定範囲を超える電流を長時間入力しないでください。本器を破損する恐れがあります。

⚠ 注意

- 直射日光や高温、多湿、結露するような環境下での、保存や使用はしないでください。変形、絶縁劣化を起こし、仕様を満足しなくなります。
- 本器を落下させたり、衝撃を加えないでください。クランプセンサの突き合わせ面が損傷し、測定に悪影響を及ぼします。
- クランプセンサ先端部に異物等を挟んだり、クランプセンサの隙間に物を差し込んだりしないでください。センサ特性の悪化、開閉動作不具合の原因になります。
- クランプセンサ部突き合わせ面にゴミなどが付着した場合は、測定に影響がでますので、柔らかい布で軽くふき取ってください。
- ケーブル類の被覆に損傷を与えないため、踏んだり挟んだりしないでください。
- 断線による故障を防ぐため、ケーブルの付け根を折ったり引っ張ったりしないでください。

注記

トランスや大電流路など強磁界の発生している近く、また無線機など強電界の発生している近くでは、正確な測定ができない場合があります。

使用前の確認

⚠ 警告


ケーブルの被覆が破れたり、金属が露出していないか、使用する前に確認してください。損傷がある場合は、感電事故になるので、お買上店（代理店）か最寄りの営業所にご連絡ください。

仕様

定格一次電流	AC1500 A
CT 比	10 : 1
確度保証温湿度範囲	23±5°C, 80%rh 以下 (結露しないこと)
確度保証期間	1 年間
振幅確度	±1.5% rdg. (45 ~ 66 Hz)
振幅周波数特性	±2.0% rdg. 20 Hz ~ 5 kHz (確度からの偏差)
位相確度	±1.0° 以内 (45 Hz ~ 66 Hz)
位相周波数特性	±1.0° 以内 20 Hz ~ 5 kHz (確度からの偏差)
導体位置の影響	±1.5% 以内 (中心からの偏差)
外部磁界の影響	AC400 A/m の外部磁界に対して 1 A 相当以下
最大入力電流	AC1000 A 連続, AC1500 A (5 分間)
温度係数	0.02%rdg./°C
使用温湿度範囲	0 ~ 50°C, 80%rh 以下 (結露しないこと)
保存温湿度範囲	-10 ~ 60°C, 80%rh 以下 (結露しないこと)
使用場所	高度 2000 m 以下, 屋内
耐電圧	AC5312 Vrms 15 秒間 (ケース - コア間)
対地間最大定格電圧	AC600 Vrms 以下
製品保証期間	1 年間
適合規格	(安全性) EN61010 タイプ A 電流センサ 測定カテゴリ III, 汚染度 2 (予想される過渡過電圧 6000 V)
測定可能導体径	φ55 mm 以下, 80 × 20 mm プスパー
二次コイル内径	内径約 27 mm × 27 mm
ケーブル長	約 3 m
外形寸法	約 99.5W 5 188H 5 42D mm (突起物含まず)
質量	約 580 g
付属品	取扱説明書 1 部 マークバンド 6 個 (3 組)

rdg.: 読み値 (現在測定中の値、測定器が現在指示している値を表します)

各部の名称

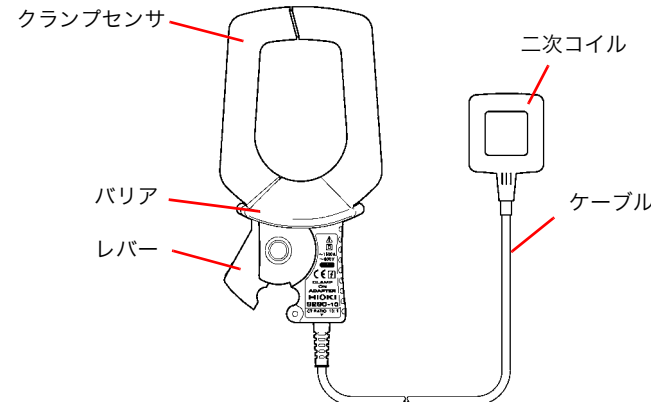


クランプセンサおよび二次コイルには、測定電流と出力電流の位相を同位相にするための電流方向マークが付いています。

測定方法

注記

導体は必ず 1 本だけクランプしてください。単相 (2 本)、三相 (3 本) を同時にクランプした場合は測定できません。

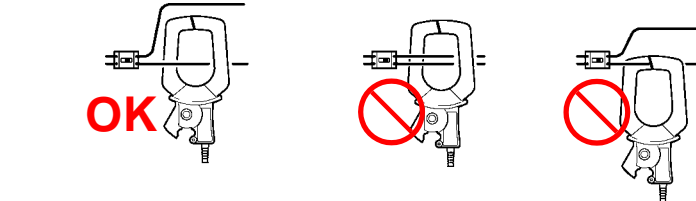


クランプする

電流方向マークを負荷側へ向ける (測定電流と出力電流の位相を同位相にするため)

- クランプセンサ部を開き、電流方向マークの矢印を負荷側に向けて、導体を 1 本だけ中央にクランプします。
- クランプセンサ部が確実に閉じていることを確認します。
- 二次コイルの窓部を、クランプセンサでクランプします。このとき、二次コイルの電流方向マークとクランプするクランプセンサの電流方向マークの向きを合わせてください。
- 指示値 × 10 倍の値が被測定電路の電流値です。

クランプセンサ、クランプ電流計との組み合わせ例

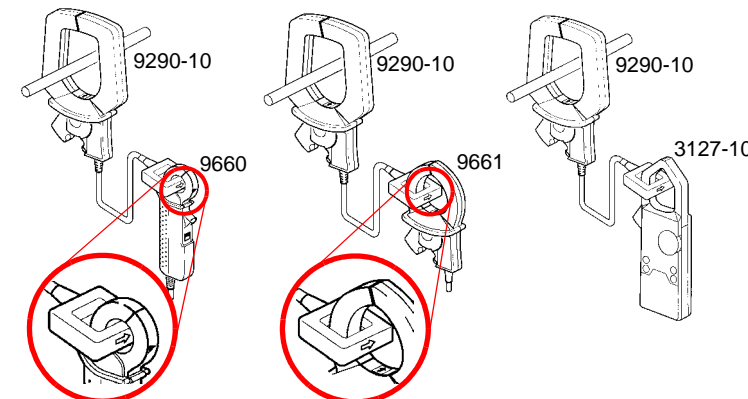

注記

二次コイルにクランプするクランプセンサの導体位置の影響を考慮する必要があります。クランプするクランプセンサの仕様をご確認ください。

9290-10

CLAMP ON ADAPTER

Instruction Manual

September 2013 Revised edition 5 Printed in Japan
9290B980-05 13-09H

HIOKI

HIOKI E. E. CORPORATION

Headquarters

81 Koizumi, Ueda, Nagano 386-1192, Japan
TEL +81-268-28-0562 FAX +81-268-28-0568
E-mail: os-com@hioki.co.jp URL http://www.hioki.com/
(International Sales and Marketing Department)

1307

For regional contact information, please go to our website at <http://www.hioki.com>.

The Declaration of Conformity for instruments that comply to CE mark requirements may be downloaded from the HIOKI website.

Warranty

Warranty malfunctions occurring under conditions of normal use in conformity with the Instruction Manual and Product Precautionary Markings will be repaired free of charge. This warranty is valid for a period of one (1) year from the date of purchase. Please contact the distributor from which you purchased the product for further information on warranty provisions.

Introduction

Thank you for purchasing the HIOKI 9290-10 CLAMP ON ADAPTER. To obtain maximum performance from the product, please read this manual first, and keep it handy for future reference.

Overview

The Model 9290-10 is a clamp-on adapter rated for 1500A AC, with a 10:1 CT ratio. In addition to the larger clamping capability, broad frequency characteristics and good phase characteristics reliably provide clamp-on Power HiTesters with expanded range and large current measurements.

Initial Inspection

When you receive the product, inspect it carefully to ensure that no damage occurred during shipping. If damage is evident, or if it fails to operate according to the specifications, contact your dealer or Hioki representative.

Maintenance and Service

- To clean the product, wipe it gently with a soft cloth moistened with water or mild detergent. Never use solvents such as benzene, alcohol, acetone, ether, ketones, thinners or gasoline, as they can deform and discolor the case.
- If the product seems to be malfunctioning, contact your dealer or Hioki representative. Pack the product carefully so that it will not be damaged during shipment, and include a detailed written description of the problem. Hioki cannot be responsible for damage that occurs during shipment.

Safety

Follow these precautions to ensure safe operation and to obtain the full benefits of the various functions.

⚠ DANGER

This product is designed to conform to IEC 61010 Safety Standards, and has been thoroughly tested for safety prior to shipment. However, mishandling during use could result in injury or death, as well as damage to the product. Be certain that you understand the instructions and precautions in the manual before use. We disclaim any responsibility for accidents or injuries not resulting directly from product defects.

Safety Symbol


	In the manual, the ⚠ symbol indicates particularly important information that the user should read before using the product. The ⚠ symbol printed on the product indicates that the user should refer to a corresponding topic in the manual (marked with the ⚠ symbol) before using the relevant function.
	Indicates a double-insulated device.
	Indicates AC (Alternating Current).
	Indicates that the instrument may be connected to or disconnected from a live circuit.

The following symbols in this manual indicate the relative importance of cautions and warnings.

- ⚠ DANGER** Indicates that incorrect operation presents an extreme hazard that could result in serious injury or death to the user.
- ⚠ WARNING** Indicates that incorrect operation presents a significant hazard that could result in serious injury or death to the user.
- ⚠ CAUTION** Indicates that incorrect operation presents a possibility of injury to the user or damage to the product.
- NOTE** Advisory items related to performance or correct operation of the product.

Measurement categories

This product complies with CAT III safety requirements. To ensure safe operation of measurement products, IEC 61010 establishes safety standards for various electrical environments, categorized as CAT II to CAT IV, and called measurement categories.

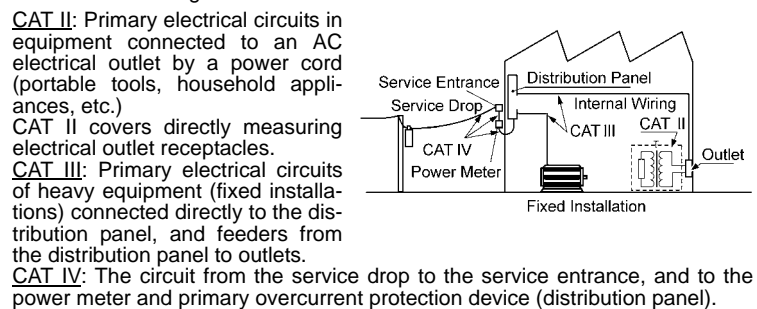

Using a measurement product in an environment designated with a higher-numbered category than that for which the product is rated could result in a severe accident, and must be carefully avoided. Use of a measurement instrument that is not CAT-rated in CAT II to CAT IV measurement applications could result in a severe accident, and must be carefully avoided.

Usage Notes

This manual contains information and warnings essential for safe operation of the product and for maintaining it in safe operating condition. Before using the product, be sure to carefully read the following safety notes.

⚠ DANGER

- To avoid short circuits and potentially life-threatening hazards, never attach the product to a circuit that operates at more than the 600V.
- This product should only be connected to the secondary side of a breaker, so the breaker can prevent an accident if a short circuit occurs. Connections should never be made to the primary side of a breaker, because unrestricted current flow could cause a serious accident if a short circuit occurs.
- To avoid electric shock, do not touch the portion beyond the protective barrier during use.

⚠ WARNING

- To avoid electric shock, do not allow the product to get wet, and do not use it when your hands are wet.
- To avoid electric shock when measuring live lines, wear appropriate protective gear, such as insulated rubber gloves, boots and a safety helmet.
- Note that the product may be damaged if current exceeding the selected measurement range is applied for a long time.

⚠ CAUTION

- Do not store or use the product where it could be exposed to direct sunlight, high temperature or humidity, or condensation. Under such conditions, the product may be damaged and insulation may deteriorate so that it no longer meets specifications.
- Be careful to avoid dropping the product or otherwise subjecting them to mechanical shock, which could damage the mating surfaces of the core and adversely affect measurement.
- Keep the clamp jaws and core slits free from foreign objects, which could interfere with clamping action.
- Keep the clamp closed when not in use, to avoid accumulating dust or dirt on the mating core surfaces, which could interfere with clamp performance.
- Avoid stepping on or pinching the cable, which could damage the cable insulation.
- To avoid damaging the cables, do not bend or pull the cables.

NOTE

Accurate measurement may be impossible in the presence of strong magnetic fields, such as near transformers and high-current conductors, or in the presence of strong electromagnetic fields such as near radio transmitters.

Preliminary Checks

⚠ WARNING

Before using the product, make sure that the insulation on the cables is undamaged and that no bare conductors are improperly exposed. Using the product in such conditions could cause an electric shock, so contact your dealer or Hioki representative for repair.


Before using the product the first time, verify that it operates normally to ensure that no damage occurred during storage or shipping. If you find any damage, contact your dealer or Hioki representative.

Specifications

Rated primary current	1500 A AC
CT ratio	10 : 1
Operating temperature and humidity for guaranteed accuracy	23±5°C (73±41°F), 80%RH or less (non-condensating)
Period of guaranteed accuracy	1 year
Amplitude accuracy	±1.5% rdg. (at 45 - 66 Hz)
Amplitude frequency characteristics	Within ±2% rdg. at 20 Hz - 5 kHz (deviation from accuracy)
Phase accuracy	Within ±1.0° (at 45 - 66 Hz)
Phase frequency characteristics	Within ±1.0° at 20 Hz - 5 kHz (deviation from accuracy)
Effect of conductor position	Within ±1.5% (deviation from center)
Effect of external electromagnetic field	1 A equivalent or less (in an AC electromagnetic field of 400 A/m)
Maximum input current	1000 A continuous, 1500 A AC (5 minutes)
Temperature coefficient	0.02%/rdg./°C
Operating Temperature & Humidity	0 to 50°C (32 - 122°F), 80%RH or less (non-condensating)
Storage Temperature & Humidity	-10 to 60°C (14 - 140°F), 80%RH or less (non-condensating)
Operating Environment	Indoors, <2000 m (6562-ft.) ASL
Dielectric strength	5312 V AC rms for 15 seconds (between case and core)
Maximum rated voltage to earth	600 V AC rms or less
Standards applying	Safety EN61010 Type A current sensor Measurement Category III, Pollution Degree 2 (Anticipated Transient Overvoltage: 6000 V)
Measurable conductor diameter	φ55 mm (2.17") or less 80 X 20 mm, Buss bars
Secondary coil inside diameter	Approx. 27 mm X 27 mm (1.06" X 1.06")
Cable length	Approx. 3 m (118.11")
Size	Approx. 99.5W X 188H X 42D mm (3.92"W X 7.40"H X 1.65"D) (excluding protrusions)
Weight	Approx. 580 g (20.5 oz.)
Accessory	Instruction Manual (1), Mark band (6, 3 sets)

rdg.:reading value (The value currently being measured and indicated on the measuring product)

Parts Names

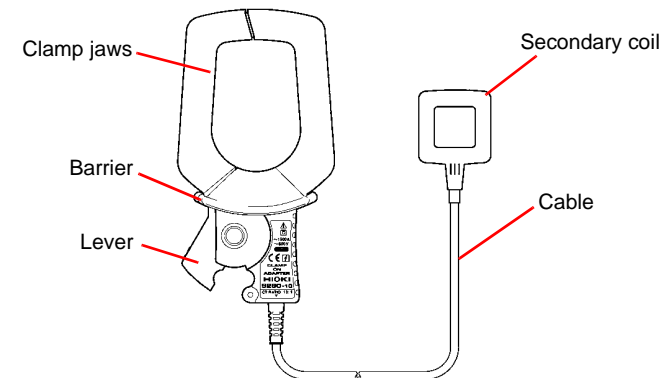


The clamp sensor and secondary coil are marked to indicate the direction of current flow, to ensure that the measurement current and output current have the same phase.


Measurement Procedures

NOTE

Attach the clamp around only one conductor. Single-phase (2-wire) or three-phase (3-wire) cables clamped together will not produce any reading.

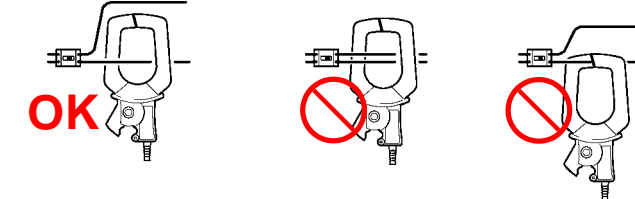


Clamp the conductor.

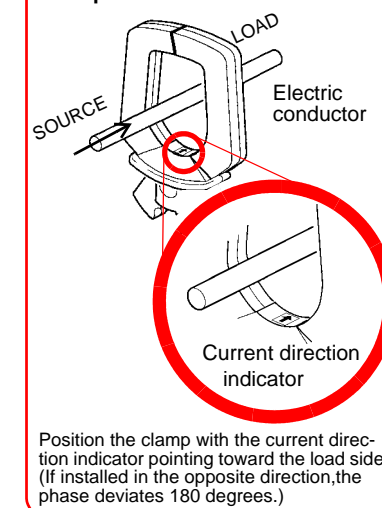

Position the clamp with the current direction indicator pointing toward the load side. (If installed in the opposite direction, the phase deviates 180 degrees.)

- Open the clamp sensor, align the current direction indicator arrow toward the load side, and clamp around one conductor.
- Make sure the clamp sensor jaws are firmly closed. Clamp the smaller clamp sensor through the opening of the secondary coil.
- In this case, be sure to align the current direction indicator arrow on the secondary coil with the indicator on the clamp sensor.
- Remember that the actual current in the circuit being measured is ten times that indicated by the measuring instrument.

Example of Combining Clamp Sensors or Clamp Meters

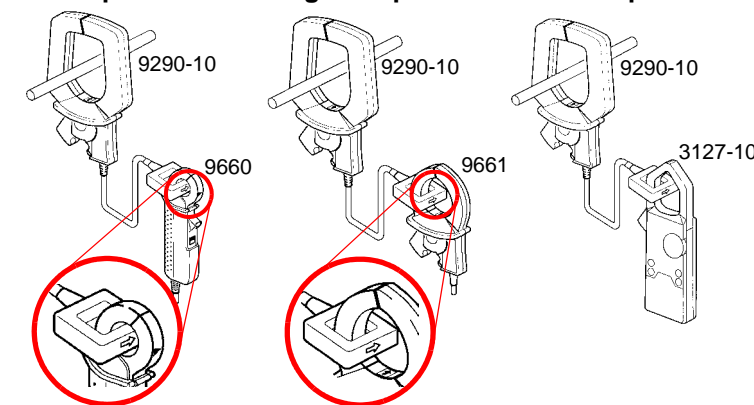

NOTE

The effect of conductor positioning of the clamp sensor clamped to the secondary coil should be considered. Please verify the specifications of the clamp sensor being used.