
NI-9476 Getting Started

2022-07-06



Contents

Before You Begin.....	3
Safety Guidelines.....	3
Safety Guidelines for Hazardous Voltages.....	3
NI-9476 with Spring Terminal Safety Voltages.....	4
NI-9476 with DSUB Safety Voltages.....	4
Safety Guidelines for Hazardous Locations.....	4
Electromagnetic Compatibility Guidelines.....	6
Special Conditions for Marine Applications.....	6
Preparing the Environment.....	7
NI-9476 Pinout.....	7
Connecting a Device.....	8
Connecting an External Power Supply.....	8
Connection Guidelines.....	9
Overvoltage Protection.....	9
High-Vibration Application Connections.....	9
I/O Protection.....	10
Protecting the Module from Flyback Voltages.....	10
Increasing Current Drive.....	10
Where to Go Next.....	11
NI Services.....	11

Before You Begin

Read the **NI-9476 Safety, Environmental, and Regulatory Information** and complete the software and hardware installation procedures in your chassis documentation.

Safety Guidelines



Caution Observe all instructions and cautions in the user documentation. Using the product in a manner not specified can damage the product and compromise the built-in safety protection.



Attention Suivez toutes les instructions et respectez toutes les mises en garde de la documentation d'utilisation. L'utilisation du produit de toute autre façon que celle spécifiée risque de l'endommager et de compromettre la protection de sécurité intégrée.

Safety Guidelines for Hazardous Voltages



Caution Ensure that hazardous voltage wiring is performed only by qualified personnel adhering to local electrical standards.



Caution Do not mix hazardous voltage circuits and human-accessible circuits on the same module.



Caution Ensure that devices and circuits connected to the module are properly insulated from human contact.



Caution When module terminals are hazardous voltage LIVE ($>42.4 V_{pk}/60 V$ DC), you must ensure that devices and circuits connected to the module are properly insulated from human contact.

NI-9476 with Spring Terminal Safety Voltages

Connect only voltages that are within the following limits.

V_{sup} -to-COM	40 V DC maximum
DO	$V_{COM} \leq V_{DO} \leq V_{sup}$
Isolation	
Channel-to-channel	None
Channel-to-earth ground	
Continuous	250 V RMS, Measurement Category II
Withstand up to 5,000 m	3,000 V RMS, verified by a 5 s dielectric withstand test

NI-9476 with DSUB Safety Voltages

Connect only voltages that are within the following limits.

V_{sup} -to-COM	40 V DC maximum
DO	$V_{COM} \leq V_{DO} \leq V_{sup}$
Isolation	
Channel-to-channel	None
Channel-to-earth ground	
Continuous	60 V DC, Measurement Category 1
Withstand up to 2,000 m	1,000 V RMS, verified by a 5 s dielectric withstand test

Safety Guidelines for Hazardous Locations

The NI-9476 is suitable for use in Class I, Division 2, Groups A, B, C, D, T4 hazardous locations; Class I, Zone 2, AEx nA IIC T4 Gc and Ex nA IIC T4 Gc hazardous locations; and nonhazardous locations only. Follow these guidelines if you are installing the NI-9476 in a potentially explosive environment. Not following these guidelines may result in serious injury or death.



Caution Do not disconnect I/O-side wires or connectors unless power has been switched off or the area is known to be nonhazardous.



Caution Do not remove modules unless power has been switched off or the area is known to be nonhazardous.




Caution Substitution of components may impair suitability for Class I, Division 2, or Zone 2.



Caution The system must be installed in an enclosure certified for the intended hazardous (classified) location, having a tool secured cover/door, where a minimum protection of at least IP54 is provided.

Special Conditions for Hazardous Locations Use in Europe and Internationally

The NI-9476 with spring terminal has been evaluated as Ex nA IIC T4 Gc equipment under DEMKO 12 ATEX 1202658X and is IECEx UL 14.0089X certified. The NI-9476 with DSUB has been evaluated as Ex nA IIC T4 Gc equipment under DEMKO 03 ATEX 0324020X and is IECEx UL 14.0089X certified. Each NI-9476 is marked  II 3G and is suitable for use in Zone 2 hazardous locations, in ambient temperatures of $-40^{\circ}\text{C} \leq T_a \leq 70^{\circ}\text{C}$. If you are using the NI-9476 in Gas Group IIC hazardous locations, you must use the device in an NI chassis that has been evaluated as Ex nC IIC T4, Ex IIC T4, Ex nA IIC T4, or Ex nL IIC T4 equipment.



Caution Transient protection shall be provided that is set at a level not exceeding 140% of the peak rated voltage value of 85 V at the supply terminals to the equipment.



Caution The system shall only be used in an area of not more than Pollution Degree 2, as defined in IEC/EN 60664-1.



Caution The system shall be mounted in an ATEX/IECEx-certified enclosure with a minimum ingress protection rating of at least IP54 as defined in IEC/EN 60079-15.



Caution The enclosure must have a door or cover accessible only by the use of a tool.

Electromagnetic Compatibility Guidelines

This product was tested and complies with the regulatory requirements and limits for electromagnetic compatibility (EMC) stated in the product specifications. These requirements and limits provide reasonable protection against harmful interference when the product is operated in the intended operational electromagnetic environment.

This product is intended for use in industrial locations. However, harmful interference may occur in some installations, when the product is connected to a peripheral device or test object, or if the product is used in residential or commercial areas. To minimize interference with radio and television reception and prevent unacceptable performance degradation, install and use this product in strict accordance with the instructions in the product documentation.

Furthermore, any changes or modifications to the product not expressly approved by National Instruments could void your authority to operate it under your local regulatory rules.

Special Conditions for Marine Applications

Some products are approved for marine (shipboard) applications. To verify marine approval certification for a product, visit ni.com/product-certifications, search by model number, and click the appropriate link.



Notice In order to meet the EMC requirements for marine applications, install the product in a shielded enclosure with shielded and/or filtered power and input/output ports. In addition, take precautions when designing, selecting, and installing measurement probes and cables to ensure that the desired EMC performance is attained.

Preparing the Environment

Ensure that the environment in which you are using the NI-9476 meets the following specifications.


Operating temperature (IEC 60068-2-1, IEC 60068-2-2)	-40 °C to 70 °C
Operating humidity (IEC 60068-2-78)	10% RH to 90% RH, noncondensing
Pollution Degree	2
Maximum altitude	
NI-9476 with spring terminal	5,000 m
NI-9476 with DSUB	2,000 m

Indoor use only.



Note Refer to the device datasheet on ni.com/manuals for complete specifications.

NI-9476 Pinout

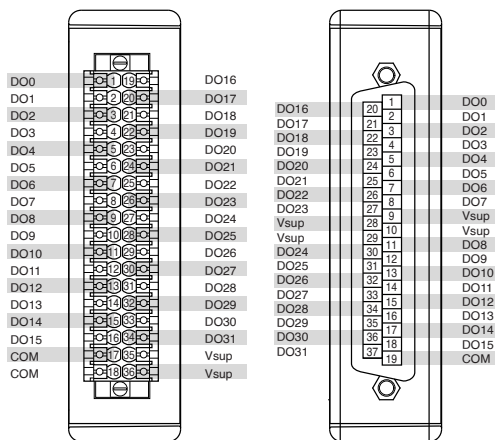

Signal	Description
COM	Common reference connection
DO	Digital output signal connection
V _{sup}	Voltage supply input connection

Table 1. Signal Descriptions

Connecting a Device

Connect the device to DO and COM, and connect the external power supply to V_{sup} and COM.



Note When DO is off, DO is not connected to COM. For devices with large source impedances, you must use a pull-down resistor between DO and COM. Visit ni.com/info and enter the Info Code CSeriesDOPulseGen for more information.

Connecting an External Power Supply

You must connect an external power supply with a 6 V DC to 36 V DC voltage range to the NI-9476. This power supply provides the current for the devices you connect to the module. You can connect only one external voltage supply to the NI-9476.

1. Connect the positive lead of the power supply to V_{sup} .
2. Connect the negative lead of the power supply to COM.



Caution Do not remove or insert modules if the external power supply connected to the V_{sup} and COM pins is powered on.

Connection Guidelines

- Make sure that devices you connect to the NI-9476 are compatible with the module specifications.
- You must use 2-wire ferrules to create a secure connection when connecting more than one wire to a single terminal on the NI-9476.
- For the NI-9476 with spring terminal, push the wire into the terminal when using a solid wire or a stranded wire with a ferrule.
- For the NI-9476 with spring terminal, open the terminal by pressing the push button when using stranded wire without a ferrule.
- For CAT II measurements, you must use a power supply with isolated DC outputs.

Overvoltage Protection

The NI-9476 provides overvoltage protection between any two inputs.



Note Refer to the device datasheet on ni.com/manuals for more information about overvoltage protection.

High-Vibration Application Connections

If your application is subject to high vibration, NI recommends that you use the NI-9940 backshell kit to protect connections to the NI-9476 with spring terminal.

I/O Protection

The NI-9476 is protected against overcurrent, inrush, and short-circuit conditions in accordance with IEC 61131-2.

Each channel on the NI-9476 has circuitry that protects it from voltage and current surges resulting from short circuits.




Caution The NI-9476 can be damaged under overvoltage and reverse bias voltage conditions. Check the voltage specifications for all devices that you connect to the NI-9476.

Excessive current through a DO pin causes the channel to go into an overcurrent state. In an overcurrent state, the channel cycles off and on until the short circuit is removed or the current returns to an acceptably low level.

Each channel has a status line that indicates in software whether the channel is in an overcurrent state.

Protecting the Module from Flyback Voltages

Install an external flyback diode if the NI-9476 is switching an inductive or energy-storing device such as a solenoid, motor, or relay, and the device does not have flyback protection.

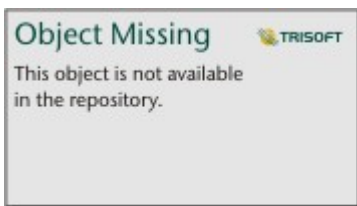


Increasing Current Drive

Each channel has a continuous output current of 250 mA. If you want to increase the output current to a device, you can connect any number of channels together in parallel. For example, if you want to drive 1 A of current, connect DO<0..3> in parallel. You must turn all parallel channels on and off simultaneously so that the current on any single channel cannot exceed the 250 mA rating.



Where to Go Next

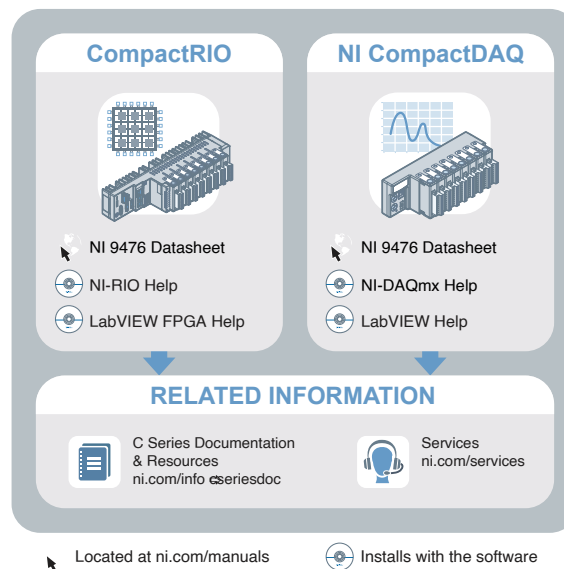

NI Services

Visit ni.com/support to find support resources including documentation, downloads, and troubleshooting and application development self-help such as tutorials and examples.

Visit ni.com/services to learn about NI service offerings such as calibration options, repair, and replacement.

Visit ni.com/register to register your NI product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

NI corporate headquarters is located at 11500 N Mopac Expwy, Austin, TX, 78759-3504, USA.