
NI-9229 Getting Started

2022-07-06



Contents

Overview.....	3
Safety Guidelines.....	3
NI-9229 with Screw Terminal Safety Voltages.....	3
NI-9229 with BNC Safety Voltages.....	4
Safety Guidelines for Hazardous Voltages.....	4
Safety Guidelines for Hazardous Locations.....	5
Electromagnetic Compatibility Guidelines.....	7
Cable Requirements for EMC Compliance.....	7
Special Conditions for Marine Applications.....	8
Preparing the Environment.....	8
NI 9229 Pinout.....	9
Grounded Connections.....	9
Floating Connections.....	10
NI-9229 Connection Guidelines.....	10
Wiring for High-Vibration Applications.....	10
Overvoltage Protection.....	10
Where to Go Next.....	10
NI Services.....	11

Overview

This document explains how to connect to the NI-9229.



Note Before you begin, read the **NI-9229 Safety, Environmental, and Regulatory Information** document on ni.com/manuals and complete the software and hardware installation procedures in your chassis documentation.



Note The guidelines in this document are specific to the NI-9229. The other components in the system might not meet the same safety ratings. Refer to the documentation for each component in the system to determine the safety and EMC ratings for the entire system.

Safety Guidelines



Caution Observe all instructions and cautions in the user documentation. Using the product in a manner not specified can damage the product and compromise the built-in safety protection.



Attention Suivez toutes les instructions et respectez toutes les mises en garde de la documentation d'utilisation. L'utilisation du produit de toute autre façon que celle spécifiée risque de l'endommager et de compromettre la protection de sécurité intégrée.

NI-9229 with Screw Terminal Safety Voltages

Connect only voltages that are within the following limits:

Isolation

Channel-to-channel

Continuous	250 V RMS, Measurement Category II
Withstand	1,390 V, verified by a 5 s dielectric withstand test

Channel-to-earth ground

Continuous	250 V RMS, Measurement Category II
Withstand	2,300 V, verified by a 5 s dielectric withstand test

Explosive atmospheres

Channel-to-channel	60 V DC, Measurement Category I
Channel-to-earth ground	60 V DC, Measurement Category I

NI-9229 with BNC Safety Voltages

Connect only voltages that are within the following limits:

Isolation

Channel-to-channel

Continuous	60 V DC, Measurement Category I
Withstand	1,000 V, verified by a 5 s dielectric withstand test

Channel-to-earth ground

Continuous	60 V DC, Measurement Category I
Withstand	1,000 V, verified by a 5 s dielectric withstand test

Safety Guidelines for Hazardous Voltages

If hazardous voltages are connected to the product, take the following precautions. A hazardous voltage is a voltage greater than:

- 30 V RMS, 42.4 V peak, or 60 V DC in DRY LOCATIONS
- 16 V RMS, 22.6 V peak, or 35 V DC in WET LOCATIONS



Caution Ensure that hazardous voltage wiring is performed only by qualified personnel adhering to local electrical standards.



Attention S'assurer que le câblage à tension dangereuse est effectué par du personnel qualifié respectant les normes électriques locales.



Caution Do not mix hazardous voltage circuits and human-accessible circuits on the same product.



Attention Ne pas combiner des circuits avec des tensions dangereuses et des circuits accessibles aux personnes sur le même produit.



Caution When product terminals are hazardous voltage LIVE, you must ensure that devices and circuits connected to the product are properly insulated from human contact.



Attention Lorsqu'une haute tension dangereuse est appliquée aux bornes du produit, vous devez vous assurer que les appareils et les circuits auxquels il est connecté sont correctement isolés de tout contact humain.



Caution You must use the NI-9971 connector backshell kit to ensure that the terminals are not accessible.

Safety Guidelines for Hazardous Locations

The NI-9229 is suitable for use in Class I, Division 2, Groups A, B, C, D, T4 hazardous locations; Class I, Zone 2, AEx nA IIC T4 Gc and Ex nA IIC T4 Gc hazardous locations; and nonhazardous locations only. Follow these guidelines if you are installing the

NI-9229 in a potentially explosive environment. Not following these guidelines may result in serious injury or death.



Caution Do not disconnect I/O-side wires or connectors unless power has been switched off or the area is known to be nonhazardous.



Caution Do not remove modules unless power has been switched off or the area is known to be nonhazardous.



Caution Substitution of components may impair suitability for Class I, Division 2, or Zone 2.




Caution The system must be installed in an enclosure certified for the intended hazardous (classified) location, having a tool secured cover/door, where a minimum protection of at least IP54 is provided.



Caution For Division 2 and Zone 2 applications, connected signals must be within the following limits.

Capacitance	0.2 μ F maximum
-------------	---------------------

Special Conditions for Hazardous Locations Use in Europe and Internationally

The NI-9229 has been evaluated as Ex nA IIC T4 Gc equipment under DEMKO 07ATEX 0626664X and is IECEx UL 14.0089X certified. Each NI-9229 is marked  II 3G and is suitable for use in Zone 2 hazardous locations, in ambient temperatures of $-40\text{ }^{\circ}\text{C} \leq T_a \leq 70\text{ }^{\circ}\text{C}$. If you are using the NI-9229 in Gas Group IIC hazardous locations, you must use the device in an NI chassis that has been evaluated as Ex nC IIC T4, Ex IIC T4, Ex nA IIC T4, or Ex nL IIC T4 equipment.



Caution Transient protection shall be provided that is set at a level not exceeding 140% of the peak rated voltage value of 85 V at the supply terminals to the equipment.



Caution The system shall only be used in an area of not more than Pollution Degree 2, as defined in IEC/EN 60664-1.



Caution The system shall be mounted in an ATEX/IECEx-certified enclosure with a minimum ingress protection rating of at least IP54 as defined in IEC/EN 60079-15.



Caution The enclosure must have a door or cover accessible only by the use of a tool.

Electromagnetic Compatibility Guidelines

This product was tested and complies with the regulatory requirements and limits for electromagnetic compatibility (EMC) stated in the product specifications. These requirements and limits provide reasonable protection against harmful interference when the product is operated in the intended operational electromagnetic environment.

This product is intended for use in industrial locations. However, harmful interference may occur in some installations, when the product is connected to a peripheral device or test object, or if the product is used in residential or commercial areas. To minimize interference with radio and television reception and prevent unacceptable performance degradation, install and use this product in strict accordance with the instructions in the product documentation.


Furthermore, any changes or modifications to the product not expressly approved by National Instruments could void your authority to operate it under your local regulatory rules.

Cable Requirements for EMC Compliance

Select and install cables for the NI-9229 with BNC in accordance with the following requirements:

- Install a clamp-on ferrite bead (NI part number 782801-01) on the BNC cable for each channel that you are connecting to on the NI-9229 with BNC.
- Clamp-on ferrites must be connected to the BNC cable as close to the module as possible with a full turn as shown in the following figure. Placing the ferrite elsewhere on the cable noticeably impairs its effectiveness.

Figure 1. Installing a Ferrite

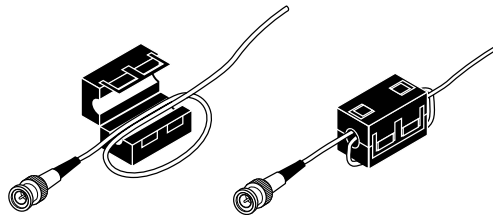

Special Conditions for Marine Applications

Some products are approved for marine (shipboard) applications. To verify marine approval certification for a product, visit ni.com/product-certifications, search by model number, and click the appropriate link.



Notice In order to meet the EMC requirements for marine applications, install the product in a shielded enclosure with shielded and/or filtered power and input/output ports. In addition, take precautions when designing, selecting, and installing measurement probes and cables to ensure that the desired EMC performance is attained.

Preparing the Environment

Ensure that the environment in which you are using the NI-9229 meets the following specifications.

Operating temperature (IEC 60068-2-1, IEC 60068-2-2)	-40 °C to 70 °C
--	-----------------


Operating humidity (IEC 60068-2-78)	10% RH to 90% RH, noncondensing
Pollution Degree	2
Maximum altitude	2,000 m

Indoor use only.



Note Refer to the device datasheet on ni.com/manuals for complete specifications.


NI 9229 Pinout

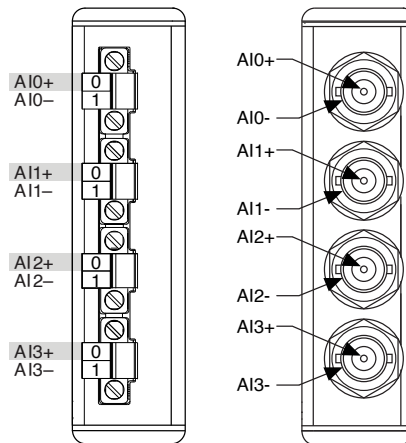


Signal	Description
AI+	Positive analog input signal connection
AI-	Negative analog input signal connection

Table 1. Signal Descriptions

Grounded Connections

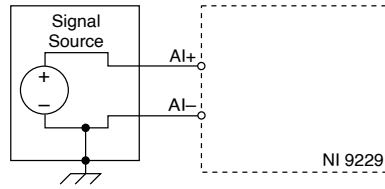

Floating Connections

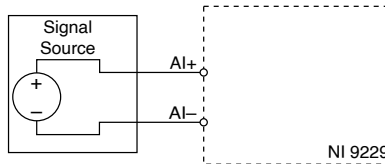

NI-9229 Connection Guidelines

- Make sure that devices you connect to the NI-9229 are compatible with the module specifications.
- You must use 2-wire ferrules to create a secure connection when connecting more than one wire to a single terminal on the NI-9229 with screw terminal.

Wiring for High-Vibration Applications

If your application is subject to high vibration, NI recommends that you follow these guidelines to protect connections to the NI-9229 with screw terminal:

- Use ferrules to terminate wires to the detachable connector.
- Use the NI-9971 backshell kit.


Overvoltage Protection

The NI-9229 provides overvoltage protection for each channel.



Note Refer to the **NI-9229 Specifications** on ni.com/manuals for more information about overvoltage protection.

Where to Go Next

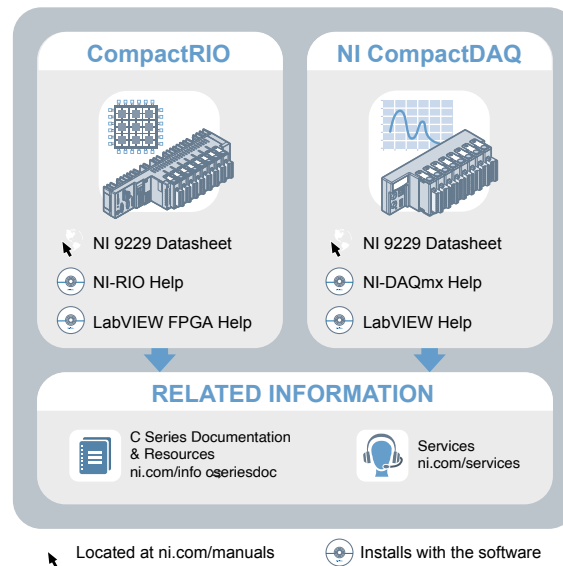

NI Services

Visit ni.com/support to find support resources including documentation, downloads, and troubleshooting and application development self-help such as tutorials and examples.

Visit ni.com/services to learn about NI service offerings such as calibration options, repair, and replacement.

Visit ni.com/register to register your NI product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

NI corporate headquarters is located at 11500 N Mopac Expwy, Austin, TX, 78759-3504, USA.